



Systematic Review

Accuracy of Invisalign® on Upper Incisors: A Systematic Review

Aline Gonçalves^{1,2}, Athénaïs Collard¹, Francisca Monteiro^{1,2-4}, David Matos¹, Óscar Carvalho^{1,2,4}, Rui Azevedo^{1,5}, Filipe S. Silva^{1,2,4}, Teresa Pinho^{1,6}

¹UNIPRO - Oral Pathology and Rehabilitation Research Unit, University Institute of Health Sciences (IUCS), CESPU, Gandra, Portugal

²Center for Microelectromechanical Systems (CMEMS), University of Minho, Campus Azurém, Guimarães, Portugal

³Life and Health Sciences Research Institute (ICVS), Medical School, University of Minho, Campus Gualtar, Braga, Portugal

⁴LABBELS - Associate Laboratory, Braga, Guimarães, Portugal

⁵TOXRUN, Toxicology Research Unit, University Institute of Health Sciences, CESPU, CRL, Gandra, Portugal

⁶BMC - Instituto Biologia Molecular e Celular, i3S - Inst. Inovação e Investigação em Saúde, Universidade do Porto, Porto, Portugal

Cite this article as: Gonçalves A, Collard A, Monteiro F, Matos D, Carvalho O, Azevedo R, Silva FS, Pinho T. Accuracy of Invisalign® on Upper Incisors: A Systematic Review. *Turk J Orthod*.

Main Points

- The accuracy of the tooth movements for the upper incisors ranged from 0% (when the teeth moved the opposite direction of the predicted movement) to 155.7% (when the achieved movement overcame the predicted one).
- For axial movements, the lateral incisors showed highly accurate (i.e., predictable) movements, especially in the labiolingual tip.
- For vertical movements, low accuracy was observed for intrusion, whereas the extrusion movement was proved to be highly accurate in both the central and lateral incisors.
- For horizontal movements, the central incisors presented highly accurate movements, especially in translation.
- Overall, the aligner showed good efficiency in reaching the desired movements in the upper incisors. Aligner features such as attachments and Power Ridge may be a good alternative to improve movement accuracy.

ABSTRACT

The current systematic review appraises the effectiveness of the types of tooth movements performed with Invisalign® clear aligner on the maxillary incisors. An electronic literature search of published trials was performed through PubMed, LILACS, Scopus, Cochrane Library, and Web of Science databases, and selected journals, from 2009 to 2020. Out of 291 references, five relevant publications were identified for analysis: four studies were performed retrospectively and one prospectively, all non-randomized. Despite the limited set of selected articles, the sample size is significant, with 148 subjects included in the reviewed studies involving the orthodontic treatment of upper incisors. We concluded that movements with the Invisalign® clear aligner on the upper incisors present distinct accuracy, possibly related with movement complexity; intrusion of the incisors has low accuracy (in some cases, 0% of accuracy was reported when the tooth extruded), while incisor extrusion exhibit some of the highest accuracy values reported in the included studies (45%-142%, when the achieved movement was greater than the predicted). Besides, axial (i.e., torque and tip) and horizontal (i.e., translation and rotation) movements are usually effective, with accuracy values between 39%-156% and 42%-79%, respectively. Overall, we determined that the efficiency of aligner to reach the desired movements in the upper incisors was low, as often refinements were required in the included studies. The use of aligner features must be more often considered to improve movement accuracy.

Keywords: Accuracy, efficiency, incisor, Invisalign®, tooth movement

INTRODUCTION

Invisalign® clear aligners (Align Technology Inc, CA, USA) are widely used in orthodontics nowadays, mostly in adult patients due to the improvement on aesthetics and comfort, as well as on hygiene and periodontal control.¹⁻⁴ Since its introduction in 1997 by Align Technology®, significant improvements were developed on the algorithms that can determine the necessary force systems to allow more accurate tooth movements.⁵

Some studies have been conducted to evaluate the movement accuracy (i.e., the predictability of the movement; the difference between achieved and predicted tooth position) with Invisalign® clear aligners, although yet sparse evidence exists on the topic. The current knowledge is quite limited, and conflicting results are reported among the existing data. Thereby, despite the officially reported ranges for movement efficacy reported by Invisalign®, they remain far from being consensual among orthodontic professionals. To address this issue, three systematic reviews evaluating the accuracy of Invisalign® clear aligners were published in the last five years.^{4,6,7} However, their conclusions were drawn regarding the type of movement instead of a specific tooth or tooth group. Accordingly, it is still difficult to assess specific clinical concerns such as those associated with upper incisors.

Having this in mind, the authors performed an electronic literature search to collect all the published evidence about the application of Invisalign® clear aligner to produce tooth movement in the upper incisors. Thus, this systematic review summarizes, compares and discusses the findings of different studies describing the tooth movement promoted by Invisalign® clear aligner in the upper incisors, aiming to identify the most affective parameters used so far by the clinicians. It also highlights and compare the accuracy and efficiency of the mechanisms triggered along the treatment.

METHODS

This systematic review followed the Preferred Reporting Items for Systematic reviews and Meta-Analyses checklist.⁸ The protocol was registered in the PROSPERO database (CRD42020190272).

Identification of Relevant Studies

Articles that compare the predicted and achieved incisor movements and/or that evaluate the accuracy/efficiency of the movement during an orthodontic treatment to the upper incisors using Invisalign® clear aligner were included. Importantly, only papers published after 2010 were included, since 2009 marked the introduction of Invisalign® Smart Technology, that brought optimized features to the orthodontics community, namely, the SmartTrack material, SmartForce features (including the Invisalign Power Ridge®), and the SmartStage technology.⁹⁻¹¹

The review strategy was lined up according to the Population, Intervention, Comparison, Outcomes, and Study design tool, as presented in Table 1.

Thus, the aim of this systematic review is to answer the question: "What is the current knowledge on the accuracy of various tooth movements performed on maxillary incisors with Invisalign® clear aligners?"

Information Sources and Search Strategy

The database search plan was discussed among all authors, who decided to use the following databases: PubMed, LILACS, Scopus, Cochrane Library, and Web of Science. Given the introduction of optimized aligner features by Invisalign® designed to improve tooth movement accuracy in 2009, only studies published in or after 2010 were included in this review. Also, only papers written in English, French, Spanish, or Portuguese were considered. In addition, a manual search was also conducted in orthodontic journals of interest to refine the survey.

The following search terms were used: (humans* OR adult* OR malocclusion* OR male* OR female*) AND (Invisalign OR clear aligners OR aligners OR transparent aligners OR orthodontic appliances, removable*) AND (cephalometry* OR orthodontic treatment OR treatment outcome*) AND (incisor* OR incisors).

Study Selection and Data Collection

Three reviewers (AG, AC and FM) independently selected the articles for analysis. In the case of disagreement, other authors (DM and TP) intervened. The same methodology was used to process the articles through the previously set criteria for inclusion and exclusion, after the duplicates were removed. References of selected articles were searched in detail to find potentially relevant studies.

Data collected from each article included the authors, year of publication, study design and population, a type of intervention, and main results associated with the accuracy of tooth movement produced by Invisalign® clear aligner on upper incisors (Table 2). When possible, accuracy metrics were uniformized in percentage using the ratio between predicted and achieved movements/positions.

Table 1. The PICOS strategy was applied to the current review

Categories	Applied Criteria
Population	Patients with permanent teeth undergoing treatment with Invisalign® clear aligner.
Intervention	Orthodontic treatment with Invisalign® clear aligner.
Comparison	Predicted vs achieved tooth position.
Outcomes	Clinical accuracy metrics of the tooth movements performed with Invisalign® clear aligner on upper incisors.
Study design	Controlled clinical trials (randomized or not), cohort studies, case control studies, and case series. Prospective, retrospective, and cross-sectional studies were also considered.

PICOS, Population, Intervention, Comparison, Outcomes, and Study design.

Methodological Quality Assessment

After data collection, two independent reviewers (AG and AC) evaluated the included studies according to the Risk of Bias in Non-randomized Studies - of Interventions (ROBINS-I) tool.¹² This approach is based on seven bias domains: confounding, participants selection, classification of interventions, deviations from intended interventions, missing data, measurement of outcomes, selection of the reported results, and overall bias. Bias assessments were tabulated with explanations when the studies were downgraded. Since assessments are inherently subjective and there are no strict and objective criteria to judge bias within the ROBINS-I tool, disagreements were resolved via a discussion between the two investigators. Bias was assessed per study rather than per outcome since there were no meaningful differences in bias across outcomes.

RESULTS

Study Selection

The electronic search initially identified 291 relevant articles. After 53 duplicate removal, 238 papers remained. Among these, 167 were excluded after title and abstract analysis. From these, 12 articles were selected for full-text reading, from which four studies were considered eligible for inclusion in the final analysis. One extra study was included from the reviewed literature,

resulting in a total of five studies to be included in the current systematic review. The selection process is depicted in Figure 1.

Study Profile

Five relevant publications were identified: four retrospective non-randomized studies, and one prospective non-randomized study. There were variations in the total sample size (range 20-38 patients), totaling 612 movements under study with upper incisors. Table 2 summarizes the main characteristics of the reviewed studies in a chronological order, enabling an intuitive comparison between the experiments and results.

The intervention among studies is similar, as all of them focus on the comparison of the final with the initial virtual models of the oral cavity, and the Invisalign® system only was used. We emphasize the classification of the intervention with the aligner features (i.e., auxiliary elements such as attachments and Power Ridge) used, compliance, and duration of treatment.

Accuracy results were written either as a mean accuracy percentage (i.e., ratio between achieved and predicted movements/positions)^{13,14}, or as the average difference (mean ± standard deviation) between predicted and achieved tooth positions.¹⁵⁻¹⁷ Accuracy values greater than 100% mean that the achieved exceeded the predicted movement.^{16,17} However, accuracy was deemed 0% when the achieved movement

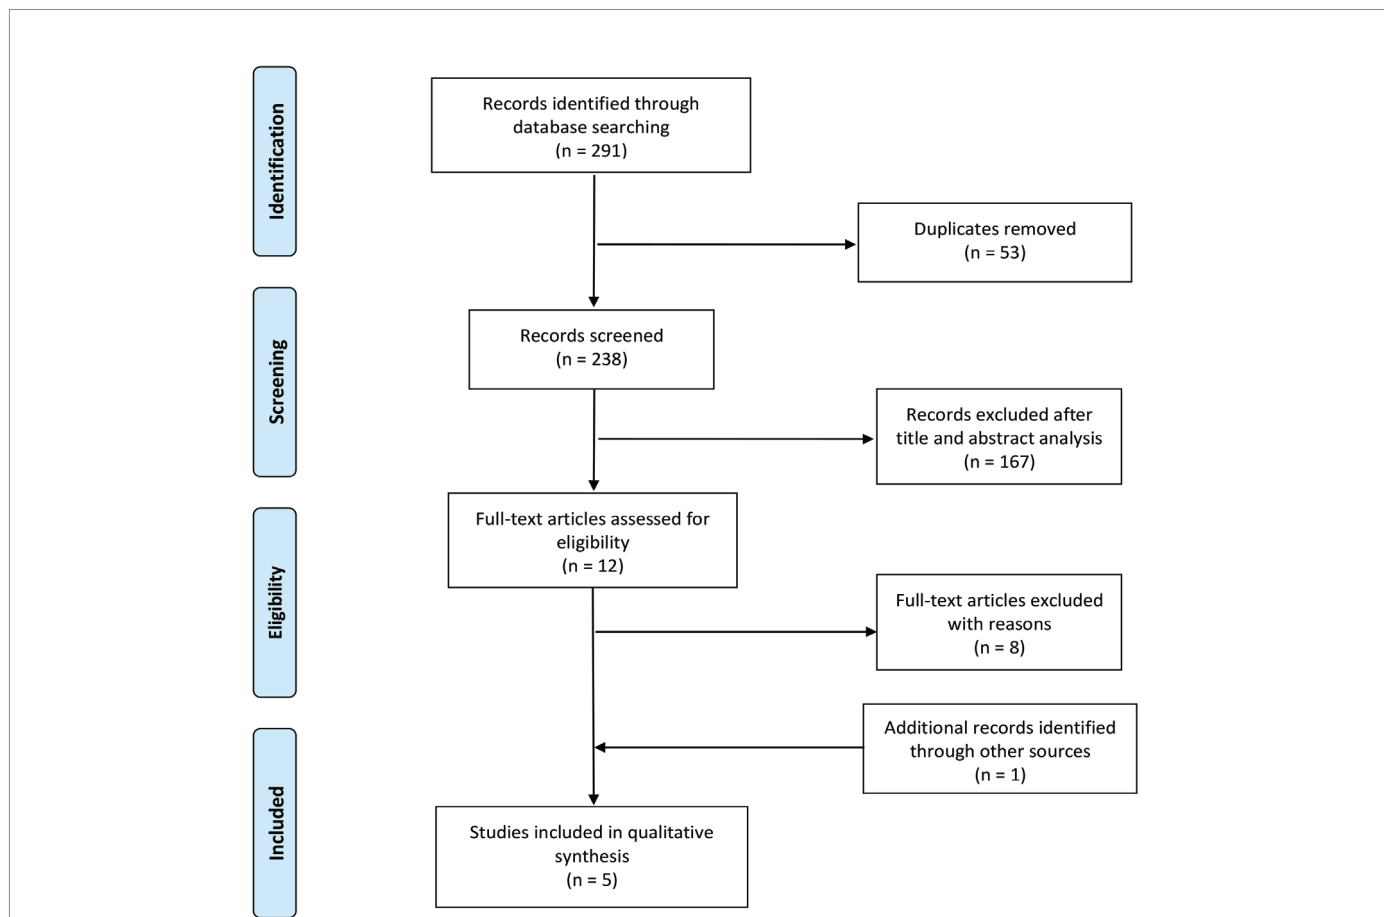


Figure 1. Flowchart from PRISMA method - articles selection process.⁸ PRISMA, Preferred Reporting Items for Systematic reviews and Meta-Analyses.

Table 2. Overview of the design and population, a type of intervention, and results of the included studies

Study	Study design	Invisalign® intervention	Results		
			Upper central incisors	Upper lateral incisors	General (other tooth movements)
Simon et al. ¹³ (2014)	Retrospective clinical study (30 patients)	<ul style="list-style-type: none"> - Time wearing the aligner: 22 h/day, except two patients who used 8 h/day - Time of aligner change: NR - Average treatment time: NR - Movement type: torque - Use of auxiliaries: torque with Power Ridge (n=7) and attachment (n=7) 	<ul style="list-style-type: none"> - Lingual torque (with attachment): 49.1% - Lingual torque (with Power Ridge): 51.5% 	NA	<ul style="list-style-type: none"> - Overall mean accuracy of tooth movement (upper incisor torque, premolar derotation and upper molar distalization): 59.3%
Grunheid et al. ¹⁵ (2017)	Retrospective cohort study (30 patients)	<ul style="list-style-type: none"> - Time wearing the aligner: NR - Time of aligner change: 2 weeks - Average treatment time: 11 ± 4 months - Movement type: torque, horizontal and vertical movement - Use of auxiliaries: no 	<ul style="list-style-type: none"> - Mesial rotation: 0.33° ± 2.80° - Lingual torque: 1.75° ± 2.86° - Distal tip: 0.42° ± 1.57° - Labial translation: 0.45 ± 0.64 mm - Mesial translation: 0.06 ± 0.40 mm - Extrusion: 0.30 ± 0.28 mm 	<ul style="list-style-type: none"> - Distal rotation: 0.70° ± 3.23° - Lingual torque: 0.08° ± 2.93° - Distal tip: 0.35° ± 2.36° - Lingual translation: 0.01 ± 0.66 mm - Mesial translation: 0.14 ± 0.39 mm - Extrusion: 0.03 ± 0.26 mm 	<ul style="list-style-type: none"> - Statistically significant differences between predicted and achieved tooth positions were found for all teeth except maxillary lateral incisors, canines, and first premolars.
Charalampakis et al. ¹⁶ (2018)	Retrospective clinical study (20 patients)	<ul style="list-style-type: none"> - Time wearing the aligner: NR - Time of aligner change: 2 weeks - Average treatment time: 12 ± 2.5 months - Movement type: horizontal, vertical displacements and mesiodistal rotations - Use of auxiliaries: no restrictions on attachment placement when needed 	<ul style="list-style-type: none"> - Mesial-distal translation: 0.24 ± 0.90 mm; 78.9% - Extrusion: -0.36 ± 0.91 mm; 128.1% - Intrusion: 1.36 ± 0.63 mm; 0% - Rotation: 2.33 ± 3.65°; 57.2% 	<ul style="list-style-type: none"> - Mesial-distal translation: 0.26 ± 0.83 mm; 77.2% - Extrusion: -0.27 ± 0.79 mm; 127.8% - Intrusion: 0.92 ± 0.70 mm; 0% - Rotation: 3.10 ± 7.34°; 66.2% 	<ul style="list-style-type: none"> - Incisor intrusion and canine rotation were the most inaccurate movements, while other tooth rotations and vertical movements were the most accurate ones.
Dai et al. ¹⁷ (2019)	Retrospective clinical study (30 patients)	<ul style="list-style-type: none"> - Time wearing the aligner: NR - Time of aligner change: every 1-2 weeks - Average treatment time: 22.3 ± 4.6 months - Movement type: torque and vertical displacement - Use of auxiliaries: torque with Power Ridge and attachments, although rare 	<ul style="list-style-type: none"> - Lingual tip: -5.16° ± 5.92°; 155.7% - Lingual translation: 2.12 ± 1.51 mm; 67.6% - Extrusion: -0.50 ± 1.17 mm; 142.4% 	NA	<ul style="list-style-type: none"> - Low accuracy of the first molar anchorage control and central incisor retraction after the first premolar extraction treatment with Invisalign.
Haoouilli et al. ¹⁴ (2020)	Prospective clinical study (38 patients)	<ul style="list-style-type: none"> - Time wearing the aligner: 22 h/day - Time of aligner change: 10 days - Movement type: torque and vertical displacement - Average treatment time: 8.5 months - Use of auxiliaries: average of six attachments 	<ul style="list-style-type: none"> - Mesial rotation: 51.3 - 61.1° - Distal rotation: 48.7 - 54.9° - Intrusion: 33.4 - 33.9% - Extrusion: 44.5 - 56.4% - Mesial tip: 47.7 - 57.5% - Distal tip: 45.5 - 49.8% - Lingual tip: 57.4 - 64.0% - Labial tip: 52.8 - 54.2% 	<ul style="list-style-type: none"> - Mesial rotation: 52.6 - 56.4% - Distal rotation: 41.8 - 48.7% - Intrusion: 36.7 - 44.6% - Extrusion: 47.1 - 53.7% - Mesial tip: 38.5 - 47.3% - Distal tip: 47.3 - 51.5% - Lingual tip: 54.4 - 57.4% - Labial tip: 61.4 - 69.9% 	<ul style="list-style-type: none"> - Overall mean accuracy for tooth movement (mesial-distal crown tip, buccal-lingual crown tip, intrusion, extrusion and rotation): 50%; - The most accurate movements were the labial crown tip of the maxillary lateral incisor, buccal-lingual lateral incisor, and rotation, whereas the least accurate movements were the mesial rotation of the mandibular first molar and intrusion of the maxillary and mandibular central incisors.

Negative values represent cases in which the achieved movement was greater than the predicted one - accuracy percentages over 100%. Accuracy values of 0% are reported when the achieved movement occurred in the opposite direction of the predicted movement. NA, not applicable.

was in the opposite direction of the desired one.¹⁶ Besides, different software was used to produce virtual models (e.g., ToothMeasure, Slicer CMF) to compare the predicted vs achieved tooth movement analysis.

Assessment of the Risk of Bias

Among the included studies, one was classified as having a low risk of bias (RoB)¹⁷ three as moderate RoB,^{13,15,16} and one study was scored with a serious risk of bias.¹⁴ See the complete data on the quality assessment in Supplementary Table S1. RoB due to missing data was considered critical, as three studies excluded individuals and reported drop-outs with missing information.^{13,14,16} Besides, three studies presented insufficient accuracy metrics, hampering result comparison.¹³⁻¹⁵

Effects of intervention on different types of movement

Torque: Four of five papers reported accuracy metrics of torque movement on upper confidence interval (CI).¹³⁻¹⁵ Accuracy percentages of CI ranged from 49.1% to 51.5%,¹³ while no information on accuracy percentages were provided for the LI. However, other authors reported a mean difference between predicted and achieved tooth positions of $1.75^\circ \pm 2.86^\circ$ for the CI, and $0.08^\circ \pm 2.93^\circ$ for the LI,¹⁵ showing great accuracy for the lingual torque in the LI.

Labiolingual tip: Regarding the labiolingual tip, the accuracy of the lingual tip ranged from 57.4% to 155.7%¹⁷ in the CI, and from 54.4% to 57.4% in the LI, while the accuracy for labial tip varied from 52.8% to 54.2% in the CI, and from 61.4% to 69.9% in the LI.¹⁴

Mesiodistal tip: The accuracy of the mesiodistal tip ranged from 45.5% to 57.5% on upper CI, and from 38.5% to 51.5% on upper LI.¹⁴ Interestingly, Haouili et al.¹⁴ found that the mesial tip was more accurate on the CI, while the tip in the distal direction showed more accuracy on the LI.

Intrusion and extrusion: Regarding the intrusion and extrusion movements, the accuracy reported by Haouili et al.¹⁴ ranged from 33.4% to 33.9% for the CI, and 36.7% to 44.6% for the LI. However, Charalampakis et al.¹⁶ observed that the vertical movement of intrusions initially predicted both for CI and LI were not accomplished, and the teeth moved toward the opposite direction (i.e., extruded). In these cases, the accuracy was deemed 0%. However, two studies reported highly accurate extrusion movements on upper CI, greater than predicted and therefore with accuracy values greater than 100%.^{16,17} Moreover, mean differences between predicted and achieved extrusion movements ranged from -0.50 ± 1.17 mm (accuracy of 142.4%)¹⁴ to 0.30 ± 0.28 mm¹⁵ for the CI, which reflect high movement accuracy, and from 0.03 ± 0.26 mm¹⁵ to 1.36 ± 0.63 mm for the LI.

Rotation: The accuracy of the rotation movement ranged from 48.7% to 61.1% on CI¹⁴ and 41.8%¹⁴ to 66.2%¹⁶ on LI. Mean differences between predicted and achieved movements varied from $0.33^\circ \pm 2.80^\circ$ ¹⁵ to $2.33^\circ \pm 1.21^\circ$ (accuracy of 57.2%)¹⁶ for the CI, whereas the same metrics for the LI ranged from $0.70^\circ \pm 3.23^\circ$

to $3.10^\circ \pm 1.48^\circ$ (accuracy of 66.1%),¹⁶ which is almost negligible and suggest a high accuracy.

Labiolingual translation: The accuracy of labial translation was assessed in two of the included articles.^{15,17} Dai et al.¹⁷ obtained a mean differences between predicted and achieved movements of 2.12 ± 1.51 mm (accuracy of 67.6%) performing labial translation of upper CI. However, Grünheid et al.¹⁵ observed a labial translation of 0.45 ± 0.64 mm and an even more accurate lingual translation of the LI of 0.01 ± 0.66 mm.

Mesiodistal translation: Only two studies evaluated the mesiodistal translation of incisors; regarding the CI, Grünheid et al.¹⁵ reported a mean difference between predicted and achieved mesial translation of 0.06 ± 0.40 mm, while Dai et al.¹⁷ observed a difference of 0.24 ± 0.90 mm between predicted and final positions. Concerning the LI, average differences of 0.14 ± 0.39 mm¹⁵ and 0.26 ± 0.03 mm (accuracy of 78.9%)¹⁷ were obtained.

DISCUSSION

Since the creation of Invisalign® clear aligner, issues associated with the movements of the upper incisors have been reported, as they fail to reach the programmed positioning.^{4,7,18} This review identifies the major limitations of the revised studies, which constitute the current literature on orthodontic treatment using aligner in upper incisors. Nevertheless, multiple movements were assessed, for which a range of mean accuracy values is presented.

Although poorly discussed among the revised studies, the aligner-wearing time is critical for movement accuracy and effectiveness. The Invisalign® treatment protocol recommends a daily use of the aligner of 22 h. Here, three of five papers do not report the instruction given to the patients concerning the aligner wearing time.¹⁵⁻¹⁷ However, the other two state that Invisalign® recommendations were followed.^{13,14} Importantly, Kravitz et al.¹⁹ described an individual case in which a patient with poor compliance to the aligner treatments (daily use of about 8 h/day) compromised the accuracy of premolar derotation. Thus, the wearing time seems to be a determinant for treatment success; and therefore, future clinical studies using aligner must clearly describe the daily time recommended for the aligner usage.

Moreover, it is important to evaluate the accuracy of the orthodontic treatments considering the use or not of aligner features. Here, only one study did not use any type of auxiliary,¹⁵ while three used attachments,^{13,14,16} and one used Power Ridge. Dai et al.¹⁷ (2019) referred that attachments and Power Ridge were rarely used to increase torque control. However, this study presented some of the greatest accuracy values for incisor lingual tip (155.7%), labiolingual translation (67.6%), and vertical movements (142.4%). Interestingly, the sample is presenting the lowest accuracy of incisor torque (49.1% and 51.5%) used

either attachments or Power Ridge.¹³ Nevertheless, the overall data suggests an increased accuracy of most of the incisor movements considered in the reviewed studies when aligner features, such as Power Ridge and attachments, are used.^{14,16,17}

Axial movements: torque and tip

Three studies evaluated the clinical torque, either lingual¹³⁻¹⁵ and labial. However, in the studies led by Simon et al.¹³ and Grünheid et al.¹⁵, the exact definition of the term “torque” is not totally clear. Statistically significant differences between the predicted and achieved tooth positions were found in both. Accuracies are only reported by Simon et al.¹³, who studied the lingual torque movement: 49.1% (with horizontal ellipsoid attachment) and 51.5% (with Power Ridge). Note that, as reported by Simon et al.¹³ and Grünheid et al.¹⁵, the reference point was determined using the virtual crown positions. Therefore, these findings may need to be interpreted with caution, as one of them considers biomechanical torque evaluation.¹⁴

To notice, Haouili et al.¹⁴ excluded the torque measurement due to the absence of radiographs evaluating the labiolingual tip, while others have been assuming the clinical torque as labiolingual tip action items.¹⁹ These findings illustrate the frequently misuse of the term “torque.” Even though, Haouili et al.¹⁴ found the highest value for labiolingual tip accuracy on LI (69.9%), although its small clinical crown has been reported as the main factor for loss of retention and movement failure throughout the treatment.²⁰⁻²⁴

Considering the labiolingual tip, the highest accuracy values were found for the lingual tip, with that of Dai et al.¹⁷ reporting a mean difference between predicted and achieved movement of $-5.16^\circ \pm 5.92^\circ$, corresponding to an accuracy of 155.7%, since the achieved movement overcame the initially predicted. It should be emphasized that the later study evaluated the accuracy of incisors' movement on a bicuspid extraction protocol.¹⁷ This rises clinical issues that might compromise the evaluation of the torque movement since, although Power Ridge has been used, torque control is more difficult to achieve due to the premolar extraction.

Haouili et al.¹⁴ also found that the labiolingual tip presented high accuracy metrics, both for CI and LI. Interestingly, the lingual tip was found to be more accurate in the CI, while the labial tip presented higher accuracy values for the LI.

Moreover, Haouili et al.¹⁴ also measured the accuracy of mesiodistal tip in the CI and LI. The authors found that the mesial tip was more accurate in the CI, whereas the distal tip presented higher accuracy in the LI. Similarly, Grünheid et al.¹⁵ reported the mean differences between predicted and achieved distal tip movements, and the results show that this movement was more accurate in the LI compared with the CI.

Vertical movements: extrusion and intrusion

Vertical movements are usually difficult to achieve, and therefore are often associated with low accuracy values, mainly with

clear aligner.^{4,16,25} However, among the reviewed studies, tooth extrusion was the most accurate movement, with two different papers reporting accuracy values greater than 100% (i.e., where the achieved movement was greater than the predicted).^{16,17} Similarly, another study reported a mean difference between the predicted and achieved movement of 0.30 ± 0.28 mm, also revealing a great accuracy of the extrusion movement. Besides, Haouili et al.¹⁴ reported accuracy values from 44.5 to 56.4% for CI, and 47.1 to 53.7% for LI, which reflects a good accuracy of the desired movement. Even though, in the referred study, a statistically significant difference between predicted and achieved tooth positioning was found for CI, but not for LI.¹⁴

In contrast, the accuracy of the intrusion movements among the included studies was typically low and, in some cases, null; specifically, Charalampakis et al.¹⁶ found that the CI and LI for which an intrusion movement was predicted actually moved toward the opposite side (i.e., extruded), and thus the accuracy of the movement was considered to be 0%. However, Haouili et al.¹⁴ observed that incisors intrusion ranged from 33.4 to 33.9% in the CI, and 36.7 to 44.6% in the LI. Among the movements studied in the work led by Haouili et al.¹⁴, intrusion presented the lowest accuracy values.¹⁶

Despite the development of optimized attachments to improve aligner grip for a more reliable intrusion, the attachment hierarchy might interfere with its placement and with the movement. Moreover, data from Charalampakis et al.¹⁶ reveal that an extrusion movement was achieved when the intrusion was programmed. The authors reported that, although tooth superimposition was based on unmovable teeth, the bite-block effect promoted some molar intrusion and it was responsible for the opposite movement observed.¹⁶ For the same reason, the extrusion movement achieved was over the expected,¹⁶ in line with what was reported by Dai et al.¹⁷

Horizontal movements: rotation, mesiodistal, and labiolingual translation

Regarding horizontal movements, translations presented higher accuracy than rotations. The greatest accuracy was found for mesiodistal translation - 78.9% for the CI and 77.2% for the LI.¹⁶ Then, lingual translation also presented good accuracy values, with the only study reporting an accuracy percentage of such movement stating an accuracy of 67.6%.¹⁷

Additionally, mesial and distal rotation movements ranged from 48.7% to 61.1% for CI and 41.8% to 66.2% for LI.^{14,16} Overall, the accuracy of mesiodistal rotation is similar comparing LI and CI. However, a lower accuracy of LI rotation could be expected due to the small clinical crown, which consequently allows a small distance between the point of application of the forces that generates smaller moments.

Overall, horizontal movements presented high accuracy metrics, with the efficiency of body movements (i.e., translation) being greater than the rotation. Specifically, the higher accuracy of rotation movement on the upper CI compared to the LI can be

explained by their flat morphology. Despite the aligner material innovations, these findings are not surprising since labial and lingual teeth provide larger surfaces for the appliance to apply forces.

Study Limitations

Very few articles have met the objective of this systematic review. As a result, a rigorous methodology for researching the biases of each selected study has been implemented. Importantly, this literature review only covers articles describing studies using clear aligner on the upper incisors and published from 2010 till the present, since 2009 marked a great innovation regarding optimized features in Invisalign aligner - the introduction of Invisalign Smart Technology.⁹⁻¹¹ Within this period, no randomized clinical trials exist on the topic. This means that no randomized experiments were ever performed on the accuracy and efficiency of tooth movements performed on maxillary incisors since the introduction of optimized aligner features. Future efforts in the field must have this into account.

Among the included studies, few samples for each incisor movement were available. Additionally, inconsistent accuracy metrics were presented among the studies; only one study reported the complete data about the predicted and achieved tooth positions,¹⁶ another study reports mean accuracy percentages without the predicted and achieved raw data,¹³ others provide the average difference between predicted and achieved tooth positions,^{15,17} while some present the maximum and minimum accuracy values.¹⁴ This really hampers the comparison of the reported results, disabling a supported and constructive search for the best orthodontic parameters. To improve comparability, when possible, the achieved and predicted movement metrics were converted into an accuracy percentage.^{16,17}

Overall, accuracy values of orthodontic movements of the upper incisors found in the literature are difficult to interpret and cross compare. Here, we uniformized the accuracy metrics reported and compiled the accuracy data (achieved vs predicted ration) into an easy-to-read and systematic table. We expect that future reports could present a complete descriptive analysis of the data, providing different accuracy metrics.

CONCLUSION

Within the limitations of this systematic review, the most important conclusions to be highlighted in the current systematic review are:

The accuracy of the tooth movements for the upper incisors ranged from 0% (when the teeth moved the opposite direction of the predicted movement) to 155.7% (when the achieved movement overcame the predicted one).

For axial movements, the lateral incisors showed highly accurate (i.e., predictable) movements, especially in the labiolingual tip;

For vertical movements, low accuracy was observed for intrusion, whereas the extrusion movement was proved to be highly accurate in both the central and lateral incisors;

For horizontal movements, the central incisors presented highly accurate movements, especially in translation;

Overall, the aligner showed good efficiency in reaching the desired movements in the upper incisors. Aligner features such as attachments and Power Ridges may be a good alternative to improve the accuracy of movement.

Ethics

Peer-review: Externally peer-reviewed.

Author Contributions: Concept - A.G.; Design - A.G.; Supervision - A.G.; Materials - A.C.; Data Collection and/or Processing - A.G., A.C.; Analysis and/or Interpretation - A.C., F.M., R.A.; Writing - A.G., A.C.; Critical Review - F.M., D.M., O.C., R.A., F.S.S., T.P.

Declaration of Interests: The authors have no conflicts of interest to declare.

Funding: This systematic review was supported by UNIPRO - Oral Pathology and Rehabilitation Research Unit in the scope of AlignAgen-GI2-CESPU-2022 and by FCT (Fundação para a Ciência e Tecnologia) through the grant 2020.09375.BD and in the scope of the project UIDB/04436/2020 and UIDP/04436/2020.

REFERENCES

- Alajmi S, Shaban A, Al-Azemi R. Comparison of Short-Term Oral Impacts Experienced by Patients Treated with Invisalign or Conventional Fixed Orthodontic Appliances. *Med Princ Pract.* 2020;29:382-388. [\[CrossRef\]](#)
- Fujiyama K, Honjo T, Suzuki M, Matsuoka S, Deguchi T. Analysis of pain level in cases treated with Invisalign aligner: Comparison with fixed edgewise appliance therapy. *Prog Orthod.* 2014;15(1):64. [\[CrossRef\]](#)
- Iliadi A, Koletsi D, Eliades T. Forces and moments generated by aligner-type appliances for orthodontic tooth movement: A systematic review and meta-analysis. *Orthod Craniofac Res.* 2019;22(4):248-258. [\[CrossRef\]](#)
- Rossini G, Parrini S, Castoroflorio T, Deregibus A, Debernardi CL. Efficacy of clear aligners in controlling orthodontic tooth movement: A systematic review. *Angle Orthod.* 2015;85(5):881-889. [\[CrossRef\]](#)
- Morton J, Derakhshan M, Kaza S, Li C. Design of the Invisalign system performance. *Semin Orthod.* 2017;23(1):3-11. [\[CrossRef\]](#)
- Papadimitriou A, Mousoulea S, Gkantidis N, Kloukos D. Clinical effectiveness of Invisalign® orthodontic treatment: a systematic review. *Prog Orthod.* 2018;19(1):37. [\[CrossRef\]](#)
- Galan-Lopez L, Barcia-Gonzalez J, Plasencia E. A systematic review of the accuracy and efficiency of dental movements with invisalign®. *Korean J Orthod.* 2019;49(3):140-149. [\[CrossRef\]](#)
- Liberati A, Altman DG, Tetzlaff J, et al. The PRISMA statement for reporting systematic reviews and meta-analyses of studies that evaluate health care interventions: explanation and elaboration. *J Clin Epidemiol.* 2009;62(10):e1-34. [\[CrossRef\]](#)
- Chang MJ, Chen CH, Chang CY, Lin JSY, Chang CH, Roberts WE. Introduction to Invisalign® Smart Technology: Attachments Design, and Recall-Checks. *J Digit Orthod.* 2019;(54):80-95. [\[CrossRef\]](#)

10. Sharma R, Rajput A, Gupta KK, Sharma H. Clear aligner: Invisalign - A review. *IP Indian J Orthod Dentofac Res.* 2020;28;4(4):173-175. [\[CrossRef\]](#)
11. Wajekar N, Pathak S, Mani S. Rise & review of invisalign clear aligner system. *IP Indian J Orthod Dentofac Res.* 2022;8(1):7-11. [\[CrossRef\]](#)
12. Sterne JA, Hernán MA, Reeves BC, et al. ROBINS-I: A tool for assessing risk of bias in non-randomised studies of interventions. *BMJ.* 2016;355:i4919. [\[CrossRef\]](#)
13. Simon M, Keilig L, Schwarze J, Jung BA, Bourauel C. Forces and moments generated by removable thermoplastic aligners: incisor torque, premolar derotation, and molar distalization. *Am J Orthod Dentofac Orthop.* 2014;145(6):728-736. [\[CrossRef\]](#)
14. Haouili N, Kravitz ND, Vaid NR, Ferguson DJ, Makki L. Has Invisalign improved? A prospective follow-up study on the efficacy of tooth movement with Invisalign. *Am J Orthod Dentofacial Orthop.* 2020;158(3):420-425. [\[CrossRef\]](#)
15. Grünheid T, Loh C, Larson BE. How accurate is Invisalign in nonextraction cases? Are predicted tooth positions achieved? *Angle Orthod.* 2017;87(6):809-815. [\[CrossRef\]](#)
16. Charalampakis O, Iliadi A, Ueno H, Oliver DR, Kim KB. Accuracy of clear aligners: A retrospective study of patients who needed refinement. *Am J Orthod Dentofacial Orthop.* 2018;154(1):47-54. [\[CrossRef\]](#)
17. Dai FF, Xu TM, Shu G. Comparison of achieved and predicted tooth movement of maxillary first molars and central incisors: First premolar extraction treatment with Invisalign. *Angle Orthod.* 2019;89(5):679-687. [\[CrossRef\]](#)
18. Lombardo L, Arreghini A, Ramina F, Huanca Ghislazoni LT, Siciliani G. Predictability of orthodontic movement with orthodontic aligners: a retrospective study. *Prog Orthod.* 2017;18(1):35. [\[CrossRef\]](#)
19. Kravitz ND, Kusnoto B, BeGole E, Obrez A, Agran B. How well does Invisalign work? A prospective clinical study evaluating the efficacy of tooth movement with Invisalign. *Am J Orthod Dentofacial Orthop.* 2009;135(1):27-35. [\[CrossRef\]](#)
20. Lacarbonara M, Accivile E, Abed MR, et al. Variable Torque Prescription: State of Art. *Open Dent J.* 2015;9(1):60-64. [\[CrossRef\]](#)
21. Burstone C, Choy K. The biomechanical foundation of clinical orthodontics. In: Burstone C, Choy K, eds. *The biomechanical foundation of clinical orthodontics.* [Internet]. First Edit. Quintessence Publishing Company 2015. <https://journals.sagepub.com/doi/pdf/10.1177/0974909820160217> [\[CrossRef\]](#)
22. Burstone C. The mechanics of the segmented arch techniques. *Angle Orthod.* 1966;(36):99-120. [\[CrossRef\]](#)
23. Gu J, Tang JS, Skulski B, et al. Evaluation of Invisalign treatment effectiveness and efficiency compared with conventional fixed appliances using the Peer Assessment Rating index. *Am J Orthod Dentofacial Orthop.* 2017;151(2):259-266. [\[CrossRef\]](#)
24. Ali SA, Miethke HR. Invisalign, an innovative invisible orthodontic appliance to correct malocclusions: advantages and limitations. *Dent Update.* 2012;39(4):254-260. [\[CrossRef\]](#)
25. Robertson L, Kaur H, Fagundes NCF, Romanyk D, Major P, Flores Mir C. Effectiveness of clear aligner therapy for orthodontic treatment: A systematic review. *Orthod Craniofac Res.* 2020;23(2):133-142. [\[CrossRef\]](#)

Supplementary Table S1. Risk of bias of observational studies by ROBINS-I quality assessment scale

Authors	Domains							Overall RoB judgment
	Preintervention		Intervention	Postintervention				
	Bias due to confounding	Bias in selecting participants for the study	Bias in classifying interventions	Bias due to deviations from intended intervention	Bias due to missing data	Bias in measuring outcomes	Bias in selecting reported result	
Simon et al. ¹³	Green	Green	Green	Green	Yellow	Green	Yellow	Yellow
Grünheid et al. ¹⁵	Green	Green	Green	Green	Green	Green	Yellow	Yellow
Charalampakis et al. ¹⁶	Green	Green	Green	Green	Yellow	Green	Green	Yellow
Dai et al. ¹⁷	Green	Green	Green	Green	Green	Green	Green	Green
Haouili et al. ¹⁴	Green	Green	Green	Green	Red	Green	Yellow	Red

Low RoB in green; Moderate RoB in yellow; and Serious RoB in red.